

System Prerequisites

Recommended configuration

Processor	Pentium® 4 or higher with support of all customary operating systems
Operating system	Microsoft Windows® 2000 / XP / Vista / Win7
Memory	512 MB RAM or higher
Monitor	VGA (1024 x 768)
Drive	CD-ROM
Input device	Mouse or compatible
Interface	USB or COM for data transmission

Install Software

- Insert the provided CD disk into CD-ROM drive.
- Double-click “XXX_VX.XX.exe” (X can be 0 to 9 or blank, indicating the software version)
- The pop-up windows will guide you through the program setup process.

Main Screen

The screenshot shows the 'Record' window with the following components:

- 1**: Main display showing 'DC 355.9 mV' with 'Auto range' below it.
- 2**: Secondary display table with columns: No., Time, Function, Value, Unit, Judge.
- 3**: Connection icon (blinking) in the top right.
- 4**: 'Pass' indicator in a green circle.
- 5**: Bar graph showing measurement data for record numbers 10 to 16.


No.	Time	Function	Value	Unit	Judge
6	09:18:21	DC	357.9	mV	pass
7	09:18:21	DC	357.7	mV	pass
8	09:18:22	DC	357.4	mV	pass
9	09:18:22	DC	357.3	mV	pass
10	09:18:23	DC	357.0	mV	pass
11	09:18:24	DC	356.7	mV	pass
12	09:18:24	DC	356.6	mV	pass
13	09:18:25	DC	356.4	mV	pass
14	09:18:25	DC	356.2	mV	pass
15	09:18:26	DC	356.0	mV	pass
16	09:18:26	DC	355.9	mV	pass

- 1** Main display screen of measurement
- 2** Secondary display screen for measurement
- 3** Blinking indicates meter is connected to the software
- 4** Data Comparison
- 5** Measurement data in graph

Using Program

Click "USB Connection" or "COM Connection" and is blinking indicates meter is successfully connected to the PC and meter will automatically start taking measurements. Primary display screen shows measurement, secondary display screen shows all measurement data.


Exit Exit and close the program

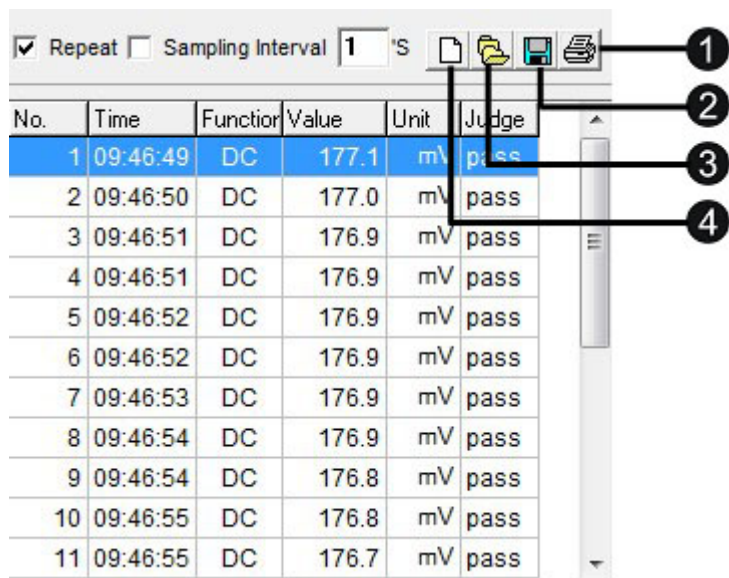

- 1 Print data
- 2 Save data (*.txt, *.xls, *.xml)
- 3 Open files (*.txt, *.xls, *.xml)
- 4 Deleting current data and create a new data.

Repeat: Tick to display every measurement with the interval you set. Un-tick “Repeat”, the secondary display screen will only show measurement result that is different from the last measured value.

Sampling Interval allows you to set the sampling intervals of measurement (1 to 9999 seconds).

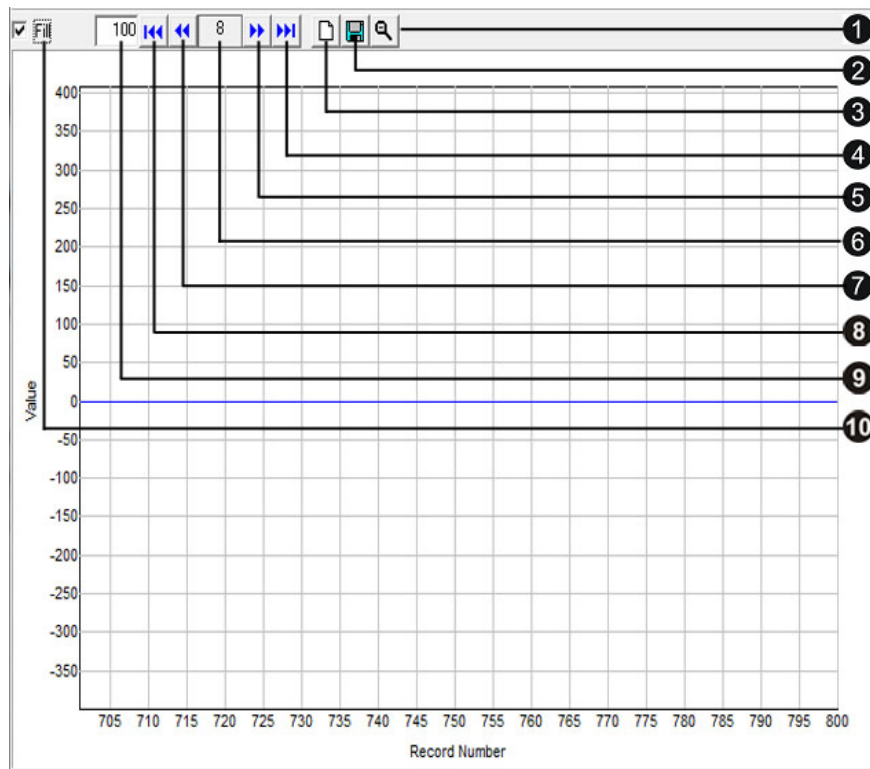

- 1 Zoom graphic
- 2 Save graph in current page as *.bmp
- 3 Deleting current data and create a new data.
- 4 Last page
- 5 Next page
- 6 Current page
- 7 Previous page
- 8 First page
- 9 Set numbers of measurement data on graph display
- 10 Fill or curve